




Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

Certificate of Analysis

Sculpt 8 mg

Report To:
Axis Research Supply Inc

Compound: Sculpt
Amount: 8 mg
Laboratory ID: V260629-33 005
Lot Number: NM62026020-01
Date Released: 7/15/2026

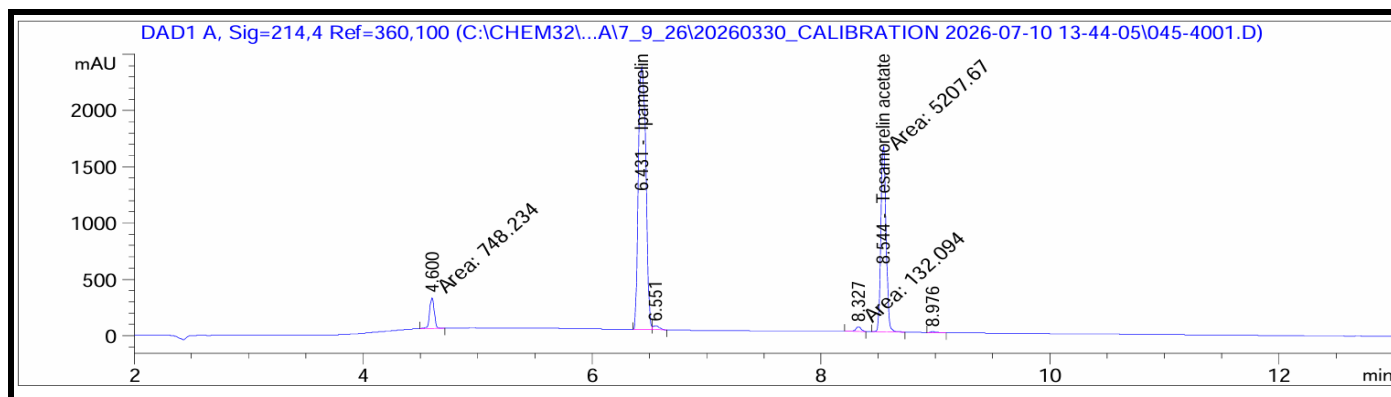

Analysis	Method	Result
Identity	HPLC-UV/VIS	Pass - Matches Ref. Standard
Chromatographic Purity	HPLC-UV/VIS	93.85% + 0.18%
Quantity: Tesamorelin	HPLC-UV/VIS	4.79 mg
Quantity: Ipamorelin	HPLC-UV/VIS	2.92 mg



Report By: Dustin Newman, Laboratory Director on 7/15/2026

Approved By: Tori Johnson, Operations Manager on 7/15/2026

Please consult A2LA Certificate #6377.01.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.



Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

Certificate of Analysis

Sculpt 8 mg

Report To:
Axis Research Supply Inc

Compound: Sculpt
Amount: 8 mg
Laboratory ID: V260629-33 005
Lot Number: NM62026020-01
Date Released: 7/15/2026

Analyte	Method	LOQ (ppm)	Result (ppm)
Arsenic (As)	ICP-MS	0.01	Not Detected
Cadmium (Cd)	ICP-MS	0.01	Not Detected
Lead (Pb)	ICP-MS	0.01	Not Detected
Mercury (Hg)	ICP-MS	0.005	Not Detected

Run ID:260713

Analysis	Method	Result
Endotoxins	LAL	Pass - <5.00 EU/mg*
Sterility	USP <71>	Pass - No Growth Detected

*Pass/Fail criteria based on the USP/FDA threshold of 5 EU/kg (350 EU total for a 70 kg adult)

Report By: Dustin Newman, Laboratory Director on 7/15/2026

Approved By: Tori Johnson, Operations Manager on 7/15/2026

ND: Non-Detect

LOD: Limit of Quantification



Please consult A2LA Certificate #6377.01.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.